
FIG. 1

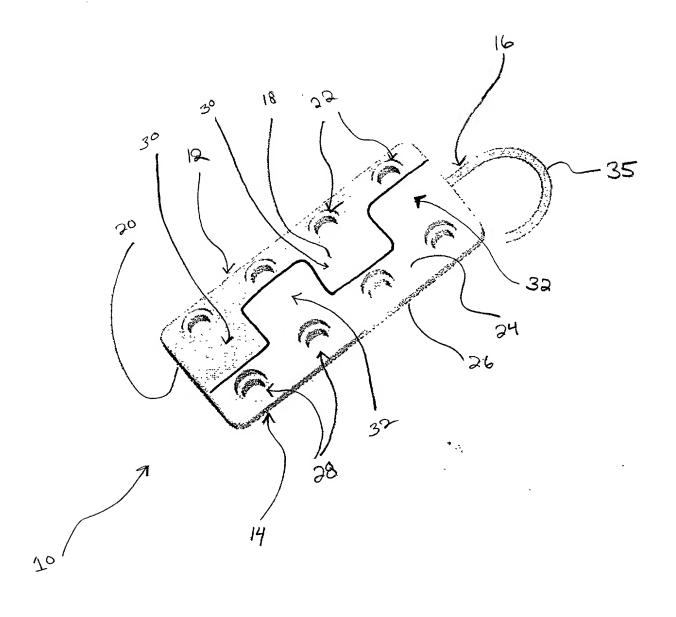

F1G. 2



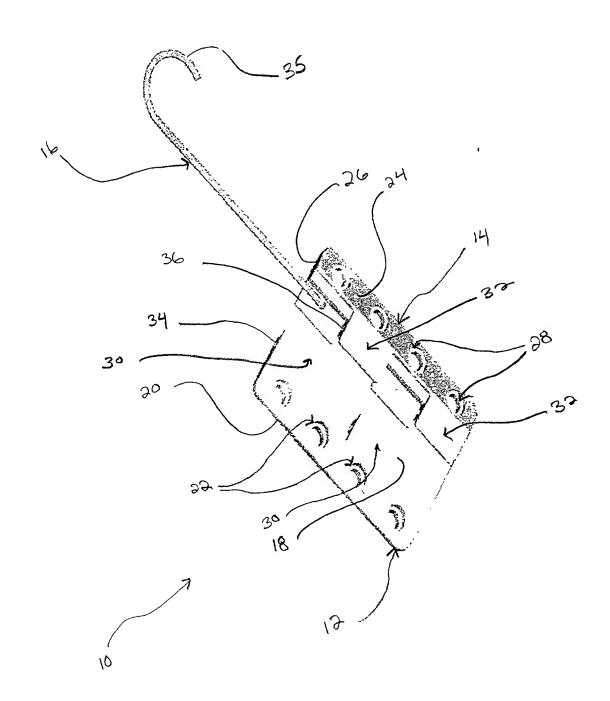


FIG. 3

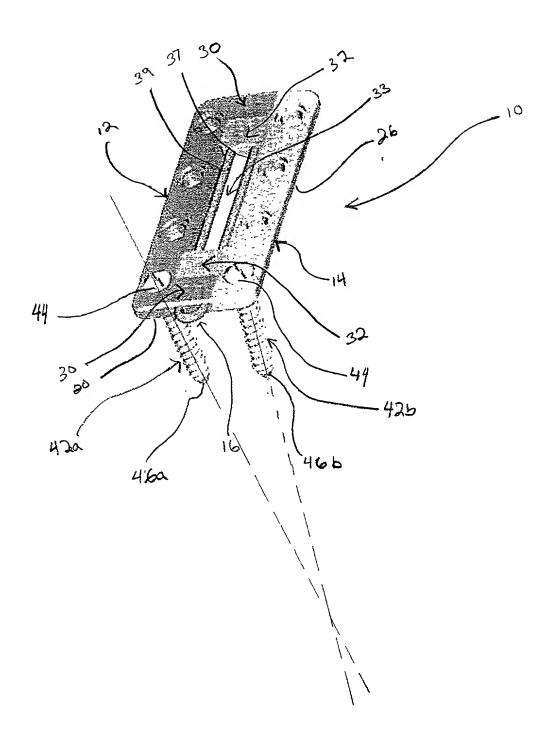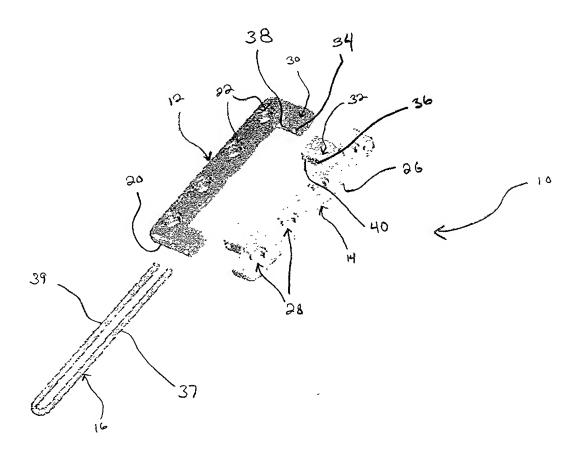

Appl Of: James P. Hearn; Filed: 2/13/02; For: Sternum Fixation Device; Atty Dkt # 8932-292; Tel: 202-496-4400; Sht 4 of 19

F16.4





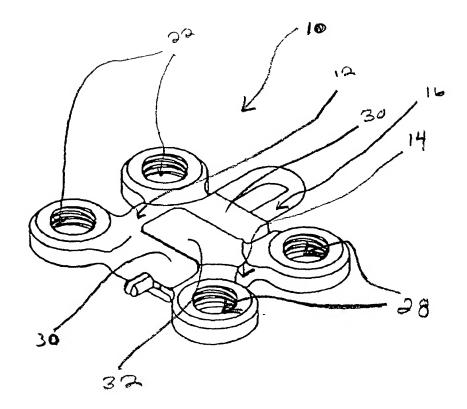



FIG. 5




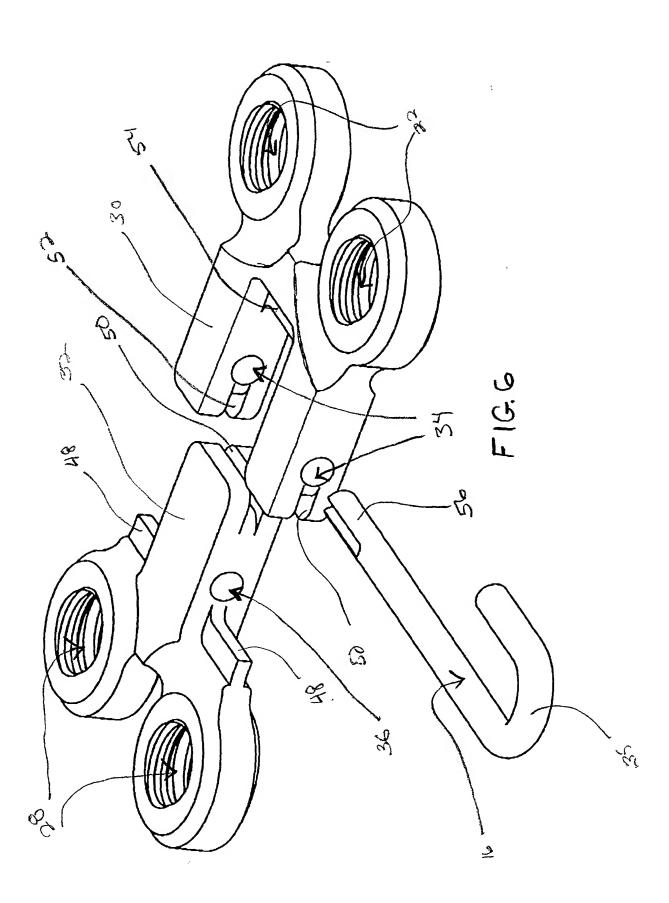

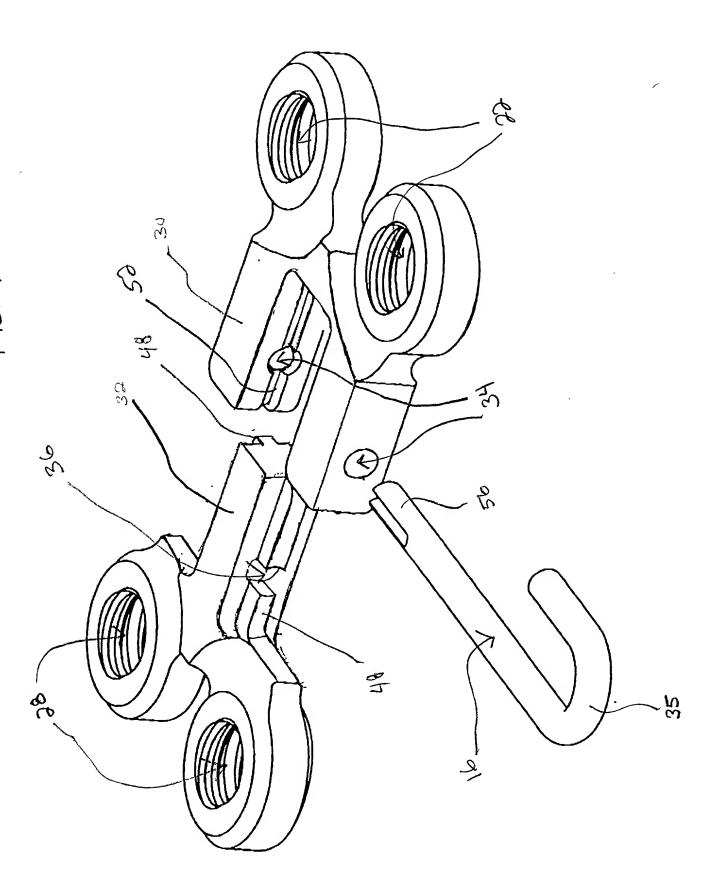


Appl Of: James P. Hearn; Filed: 2/13/02; For: Sternum Fixation Device; Atty Dkt # 8932-292; Tel: 202-496-4400; Sht 8 of 19

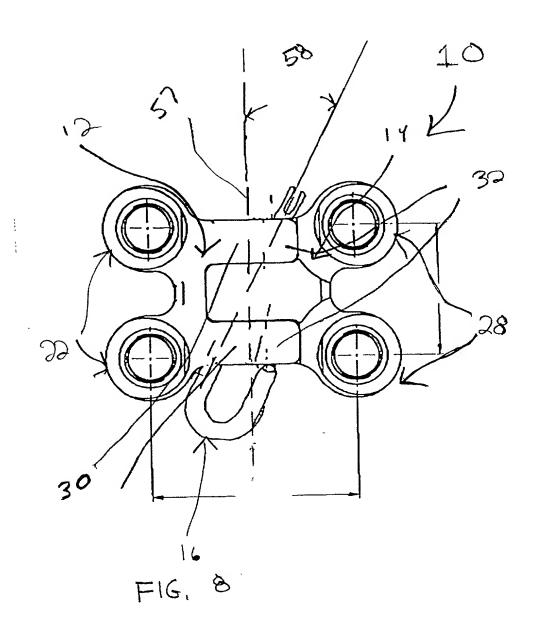


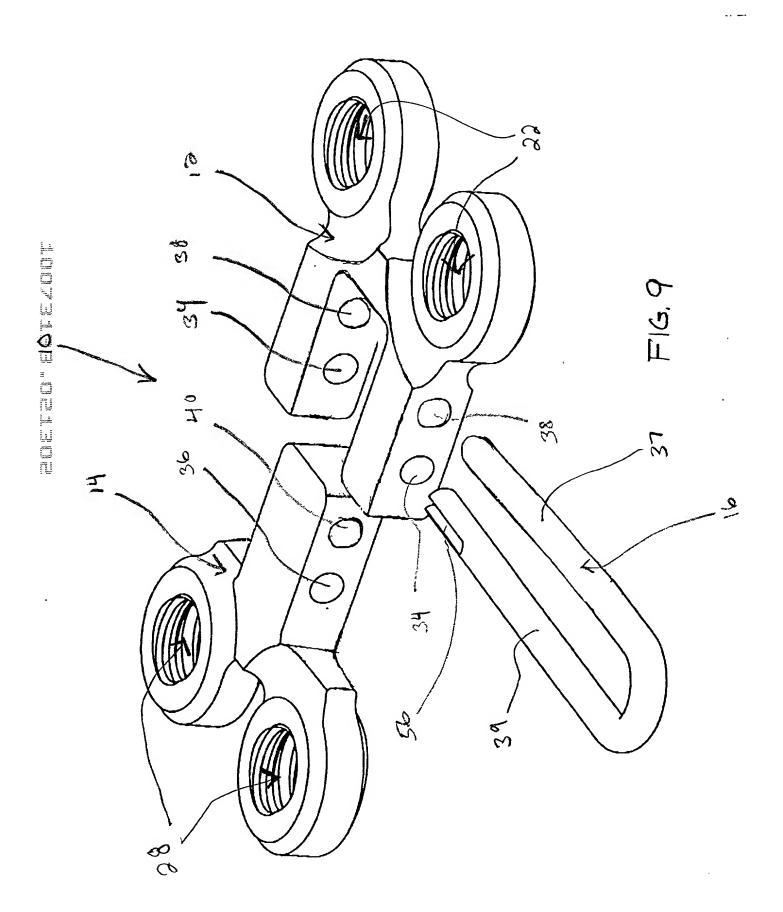


Appl Of: James P. Hearn; Filed: 2/13/02; For: Sternum Fixation Device; Atty Dkt # 8932-292; Tel: 202-496-4400; Sht 10 of 19

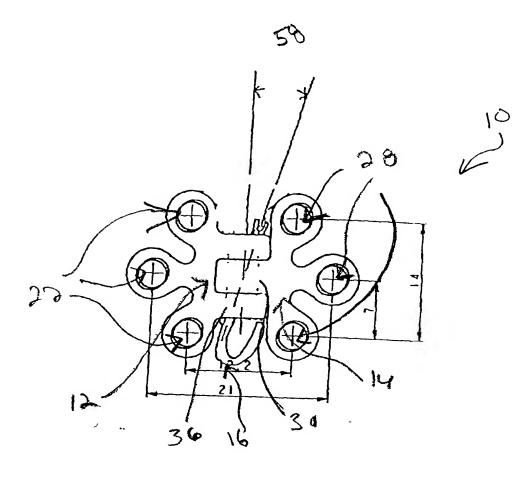


F16. 10

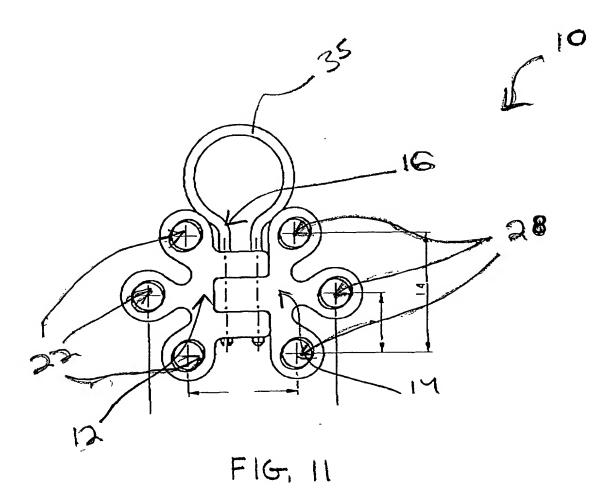


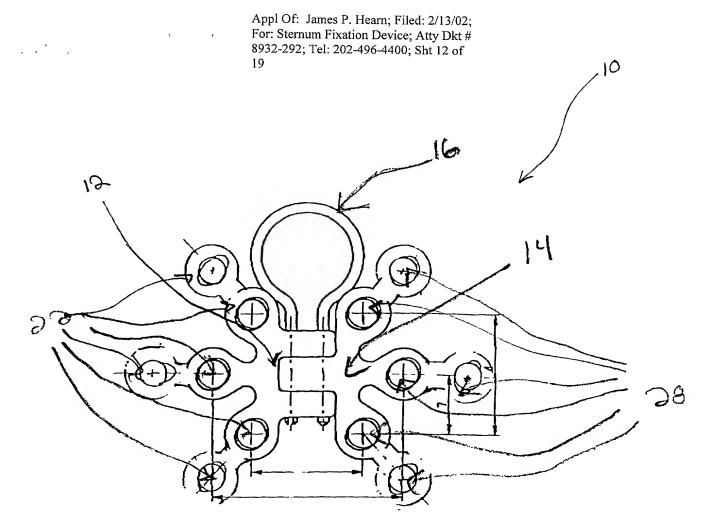


F16.12

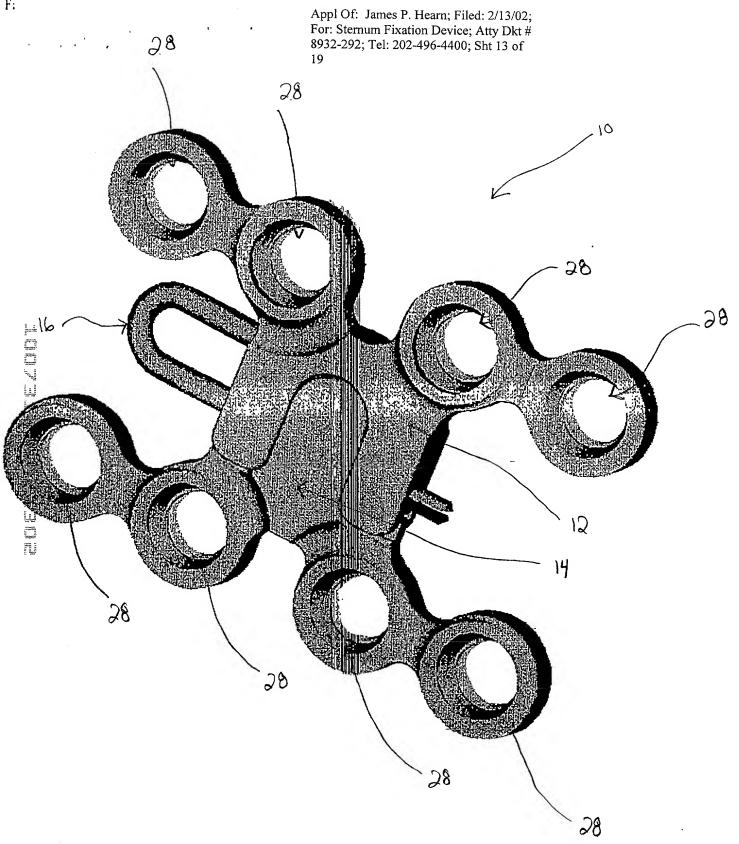


F16. 13

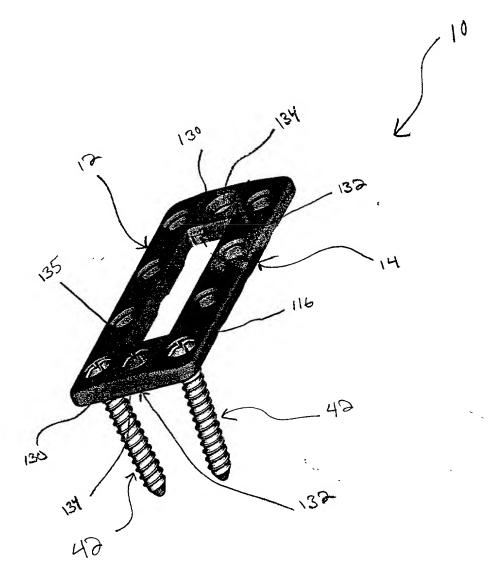


F16. 14

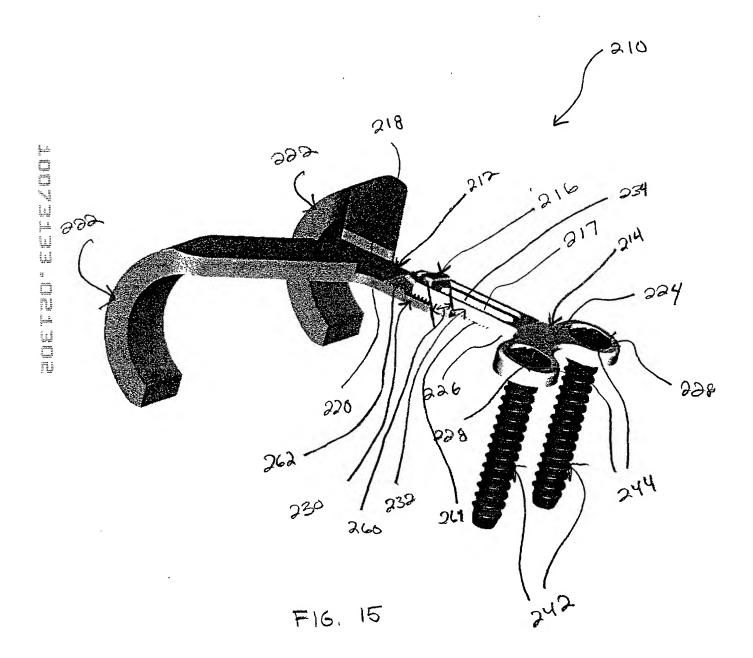

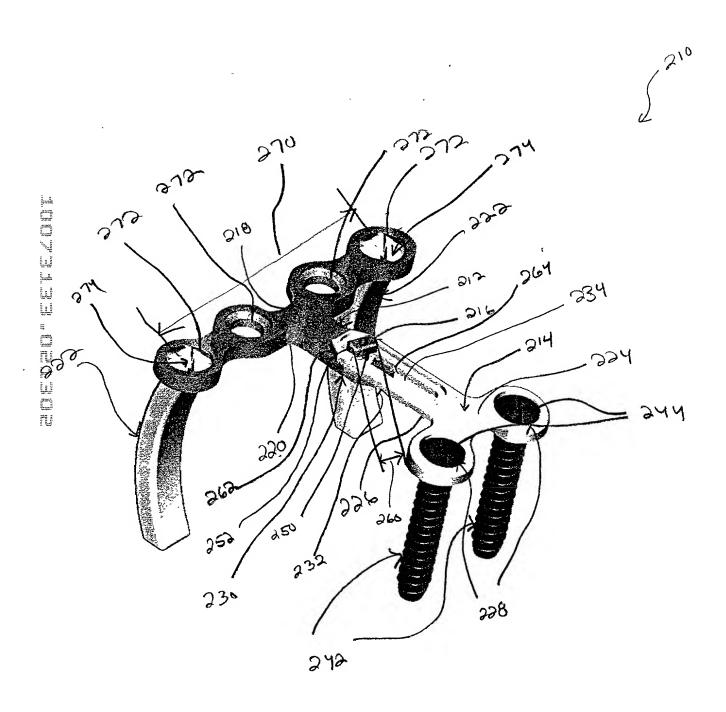


F16. 16

Appl Of: James P. Hearn; Filed: 2/13/02; For: Sternum Fixation Device; Atty Dkt # 8932-292; Tel: 202-496-4400; Sht 17 of

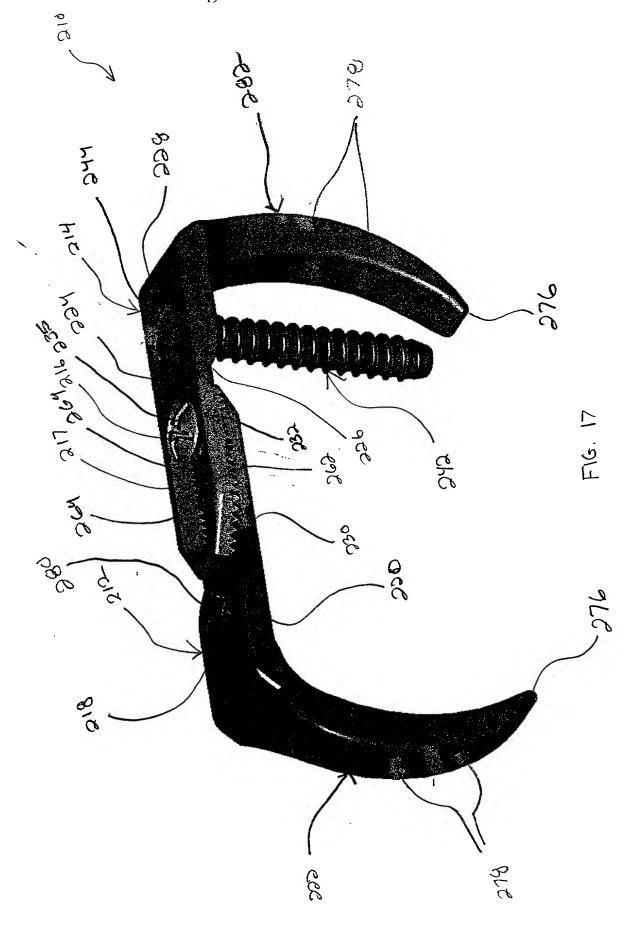

Appl Of: James P. Hearn; Filed: 2/13/02; For: Sternum Fixation Device; Atty Dkt # 8932-292; Tel: 202-496-4400; Sht 18 of 19

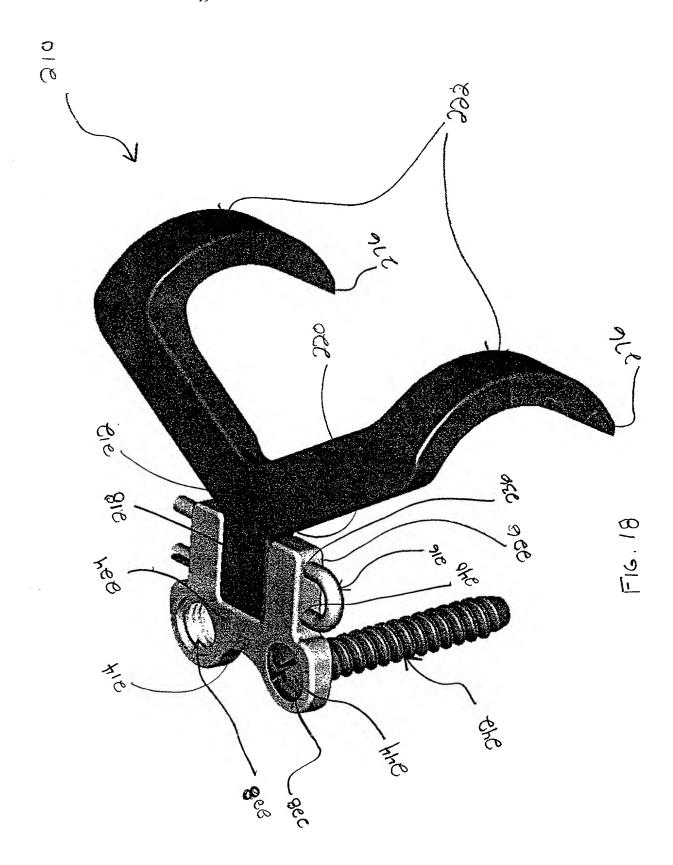

Appl Of: James P. Hearn; Filed: 2/13/02; For: Sternum Fixation Device; Atty Dkt # 8932-292; Tel: 202-496-4400; Sht 19 of

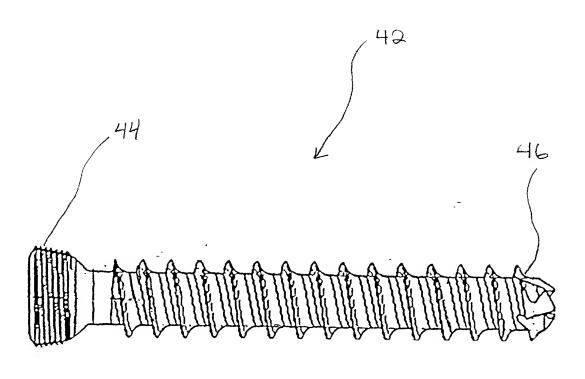


FIG. 19